



## आरोग्य विभाग

जिल्हा आरोग्य अधिकारी कार्यालय, जिल्हा परिषद, धाराशिव

दुरध्वनी क्रमांक - ०२४७२-२२०४५१



आरोग्य सेवा

ई-मेल आयडी - [dhomedistoreosbad@gmail.com](mailto:dhomedistoreosbad@gmail.com)

पिन क्रमांक ४१३५०१

जा.क्र.जिपधा/आवि/औभा/कावि/औषधीभांडार/2084/२४

दि. 11/10/२०२४

प्रति,

१.-----

२.-----

३.-----

४.-----

५. नोटीस बोर्ड

**विषय - आयुष आरोग्यवर्धीनी केंद्रासाठी आवश्यक साहित्य खरेदी करणे बाबत..**

उपरोक्त विषयानुसार आरोग्य विभाग, जिल्हा परिषद, धाराशिव अंतर्गत २ आयुष आरोग्यवर्धीनी केंद्रामध्ये सोबतच्या यादीतील आवश्यक पंचकर्म म्हणजे ईलाज बिल तदबिर (illaj-bil - tadbir = Rejemental Therapy) साहित्य/उपकरणे खरेदी करावयाचे आहे तरी आपल्या फर्मचे प्रती नगाचे सर्व करांसहित दरपत्रक देण्यात यावे.

तरी सदर दरपत्रक दिनांक - 11/10/२०२४ ते 23/10/२०२४ या कालावधीत कार्यालयीन वेळेत दुपारी ५.०० वाजे पर्यंत सिल बंद पाकीटात खालील अटी व शर्तीच्या अधिन राहून सादर करण्यात यावेत.

### अटी व शर्ती -

१. दरपत्रकातील दर हे सर्व करांसहित या कार्यालयाच्या औषधी भांडारात पोहोच करण्या पर्यंतचे असावेत.
२. वरील साहित्याचा पुरवठा केल्या नंतर देयक दोन प्रतीत या कार्यालयास सादर करण्यात यावे.
३. मागविण्यात आलेले दर पत्रक रद्द करणे किंवा मंजूर करण्याचे अधिकार या कार्यालयाने राखून ठेवलेले आहेत.
४. वरील प्रमाणे अटी व शर्ती मान्य असलेल्या फर्मनेच दर पत्रके सादर करावीत. तसेच सदर खरेदी ही तातडीची असल्यामुळे पुरवठा तात्काळ करणे आवश्यक असेल.
५. साहित्याचा पुरवठा १५ दिवसात या कार्यालयास करणे बंधनकारक असेल अन्यथा ०.५ % प्रती आठवडा दंड पुरवठा आदेशातील पुर्ण रक्कमेतुन वसूल केला जाईल याची नोंद घ्यावी.
६. दरपत्रक भरताना एका लिफाफ्यात दोन लिफाफे देण्यात यावेत लिफाफा क्र १ हा तांजीक कागदपत्रासाठी आहे व साहित्य/उपकरणाचे दर भरताना एका नगाचे सर्व करांसहित दर लिफाफा क्र २ मध्ये भरावेत. व तसे लिफाफ्यावर तांजीक लिफाफा व दराचा लिफाफा असे नाव तसेच फर्मचे नांव नमुद करणे आवश्यक आहे, लिफाफे हे सिलबंद सादर करणे आवश्यक आहे.

७. उपकरणे/साहित्य सोबत दिलेल्या स्पेसिफिकेशन प्रमाणे नसल्याचे आढळून आल्यास सदर उपकरणे/साहित्य ताब्यात घेण्यात येणार नाही याची नोंद घेण्यात यावी.

**तांजीक लिफाफा क्र १ मध्ये दयावयाच्या बंधनकारक कागदपत्राची माहिती**

१. मुंबई दुकान व संस्था अधिनियम १९४८ अंतर्गत दुकान निरीक्षक यांचे प्रमाणपत्र ज्यात धंद्याचे स्वरूप नोंदणी आहे असे वैध प्रमाणपत्र, उत्पादक असल्यास उत्पादक असल्याचे वैध प्रमाणपत्र.
२. जि.एस.टी. नोंदणी प्रमाणपत्र.
३. जि.एस.टी.कायदया प्रमाणे माहे जुन २०२४ पर्यन्त भरण्यात आलेल्या रिटर्नची प्रत.
४. पॅन कार्ड छायाप्रत
५. मागील तीन वर्षांच्या उलाढालीचे (Balance Sheet) रजिष्टर्ड चार्टर्ड अकाऊंटन्ट यांचे प्रमाणीत प्रमाणपत्र सन २०२१-२२, सन २०२२-२३ व सन २०२३-२०२४ या वर्षांचे (प्रती वर्ष किमान रु.८.०० लक्ष टर्न ओव्हर असणे आवश्यक आहे.) सोबतच्या नमुन्यात
६. मागील तीन वर्षांचे नफा व तोट्याचे (Profit & Loss Account Sheet) रजिष्टर्ड चार्टर्ड अकाऊंटन्ट यांचे प्रमाणीत प्रमाणपत्र सन २०२१-२२, सन २०२२-२३ व सन २०२३-२०२४ या वर्षांचे.
७. पुरवठाधारकांचे नांव शासनाच्या शासकिय किंवा निमशासकिय संस्थे मध्ये काढया यादीत नसल्याचे रु.५००/-च्या मुद्रांकित शुक्लावर (स्टॅप पेपर) प्रतिज्ञापत्र देणे बंधनकारक राहिल.
८. शासन निर्णय उदयोग, उर्जा व कामगार विभाग, मंजालय, मुंबई दिनांक १.१२.२०१६ नुसार हित संबंध नसल्याचे प्रमाणपत्र सोबतच्या नमुन्या नुसार देणे बंधनकारक असेल.
९. सदर उपकरणे/साहित्याचा पुरवठा शासकिय/निमशासकिय संस्थेमध्ये केल्याचे किमान प्रती वर्ष एक पुरवठा आदेशाची प्रत (सन २०२०-२१, सन २०२१-२२ व सन २०२२-२०२३)

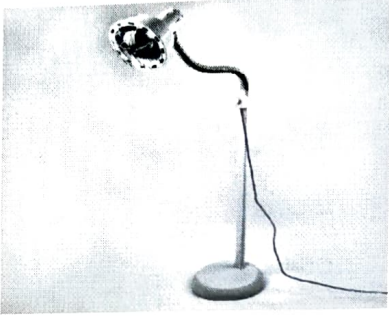

**दराचा लिफाफा क्र २ मध्ये साहित्य/उपकरणाचे दर सर्व करांसहीत खालील नमुन्यात भरण्यात यावेत**

अ.क्र	उपकरणे/साहित्याचे नांव	सर्व करांसहीत एका नगाचे दर
1	Swedana/Sudation Chamber	
2	Nadi Sweda Yantra ( 7 lirs Stainless Steel Cooker)	
3	Nadi Sweda Yantra ( 10 lirs Stainless Steel Cooker)	
4	Infrared lamp for joint swedan	
5	Basti yantra ( Niruha Basti )	
6	Basti yantra ( Anuvasan Basti )	
7	Shirodhara Yantra	
8	Shirobasti	
9	Nasya karma set	
10	Yoga Jal neti pot Plastic 200 ml	
11	Yoga neti pot Stainless Steel 500ml	
12	Yoga Mats	
13	Weighing Machines Adult Digital	
14	Weighing Machines Pediatric	
15	Swab holder	

16	Wheel chair	
17	Wooden chair	
18	Examination stool	
19	Stracher on Trolly	
20	Wheel chair for disabled patient	
21	Computer table	
22	Wooden Snehan Table	
23	Hight meter	
24	Cupping Set	

( डॉ. सतिश हरिदास )  
जिल्हा आरोग्य अधिकारी  
जिल्हा परिषद, धाराशिव

**आयुष आरोग्यवर्धीनी केंद्रासाठी आवश्यक उपकरणे व साहित्य खरेदीचे स्पेसिफिकेशन**

Name Of Items	Specification										
Swedana /Sudation Chamber ( भाप पेटी / हमाम)	स्वेदन टेबल/द्रोणी ७.५ X २.५ X ३ फुट असावे वरुन झाकण असावे, झाकण हलके असावे, शिरोभागी आधार असावा										
Nadi Sweda Yantra, 7 ltrs Stainless Steel	प्रेसर कुकर ७ लिटर										
Nadi Sweda Yantra , 10 ltrs Stainless Steel	प्रेसर कुकर १० लिटर										
<p><b>Infra Red Lamp For Joint , Swedan</b></p> <p><b>Product Specification</b></p> <table border="1" data-bbox="115 625 376 884"> <tr> <td>Usage/Application</td> <td>Hospital</td> </tr> <tr> <td>Light Source Type</td> <td>LED</td> </tr> <tr> <td>Brand</td> <td>Vision</td> </tr> <tr> <td>Material</td> <td>MS</td> </tr> <tr> <td>Positioning</td> <td>Floor Standing</td> </tr> </table> <p><b>Product Description</b></p> <p>We are counted as the foremost manufacturer and supplier of excellent quality <b>Infrared Lamp</b> that is used for to transmitting infrared radiation to the body. This lamp is manufactured using excellent quality components with the help of advanced technology. It is widely used in various medical applications in hospitals all across the country. Tested on various quality parameters, clients can avail this lamp from us from us in various power capacities at very affordable price range. this is moveable and adjustable.</p> <p><b>Features:</b></p> <ul style="list-style-type: none"> <li>• High low Intensity switch</li> <li>• Height, Angle, Direction, Adjustment can be done</li> </ul>	Usage/Application	Hospital	Light Source Type	LED	Brand	Vision	Material	MS	Positioning	Floor Standing	
Usage/Application	Hospital										
Light Source Type	LED										
Brand	Vision										
Material	MS										
Positioning	Floor Standing										
Basti Yantra (Niruha Basti) (हुकना)	स्टेन लेस स्टीलचे किमान १ लिटर द्रावण मावेल असे असावे.										
Basti Yantra (Anuvasan Basti) (हुकना)	स्टेन लेस स्टीलचे किमान २५० ते ३०० मिली द्रावण मावेल असे असावे.										
Shirodhara Yantra ( नतुले )	तांब्र धातुचे असावे,किमान २ लिटर द्रावण मावेल असे असावे.										
Shirobasti ( मस्सा )	२.५ X १२ चामडी पट्टा असावा										
Nasya Karma Set- Made up of Brass ( नतुल )											

**Yoga Jal Neti Pot (White Durable Plastic Material) 200 ml**



**Yoga Jal Neti Pot (Stainless Steel Material) 500 ml**



**Yoga Mats**

Colour	Multicolor
Brand	Generic
Material	Ethylene Vinyl Acetate



**Weighing Machine -Adult**

Personal Baby Weighing Scale for Manual Weight Upto 150 Kgs



**Weighing Machine - Pediatric**

Personal Baby Weighing Scale for Manual Weight Upto 10 Kgs with Tray (Cream)



Swab Holder

Made up of stainless Steel

Wheel Chair

**Specification**

Florence Metal Base Mid Back Mesh Revolving Office Chair (4 Color Options) (Black).



**Wooden Chair**

**Specification**

Size (LxBxH) : 20 x 18 x 36 Inch  
Material : Teak wood



Examination Stool

As Per Attached Specification

Stracher

As Per Attached Specification

Wheel Chair For Disable Patient

As Per Attached Specification

## Computer Table

### Description

stainless steel computer desk with solid top and rear rail is a perfect work and storage surface for any Office whereby a strong, easy-clean material is necessary.

Finished in brushed dull polish, the stainless steel rear rail desk comes with 304-grade stainless steel build and a 200kg payload, with a 40mm box section frame. The stainless steel adjustable feet with non-marking rubber base lend stability and strength to the unit.

With a ledge for a regular size computer tower and a keyboard shelf, also manufactured from 304 grade stainless steel, this desk is designed to house your computer safely.

### Dimensions (W x D x H unless stated)

Widths available: 1200, 1500 and 1800mm

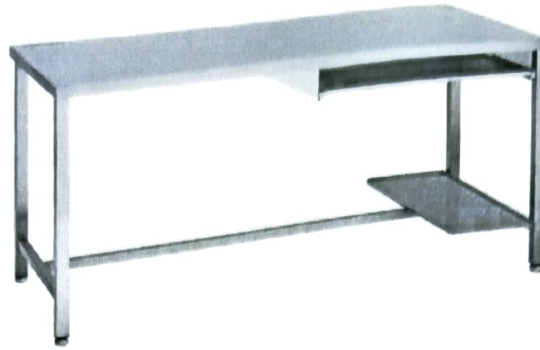
Depths: 600 and 750mm

Floor clearance: 150mm

Height: 840mm

### Specifications

- Computer desk with top and tower shelf - siliconed seal
- Fully welded 304 grade stainless steel
- Brushed dull polish finish
- Keyboard/mouse drawer
- Stainless steel adjustable feet with non-marking rubber base
- Mobile versions available



### Wooden Snehan Table

७.५ X २.५ X २.५ फुट (मुठ व्यतिरिक्त)

८.९ X २.५ X २.५ फुट (मुठ सहीत)

टेबल सागवानी असावे

### Hight Meter



### Cupping Set ( हिजामा सेट)

{Material} Made of excellent quality Plastic material-Great Other Alternate Therapy Cupping, Hijama, Suction Healing Technique tool ?

{Directions} We recommend the Acupressure half Plastic ball to be used by professionals. ?

{Indications} The therapy helps you to cure Headache, Heat stroke, Backache, Naval Imbalance and many more.



## Technical Specification of Stretcher Trolley

1	<b>Overall Size :-</b>	2100mm (L) X 560mm(W) X 820mm(H) Height from Ground level to top.
2	<b>Frame of the Trolley :</b>	<p>a) Trolley frame work, S.S tubular deep fully argon welded with vertical upright 31.75mm OD, 18SWG tubes. Tube should be reinforced at the bottom with 35mm OD, 18SWG tube for fitting the wheels.</p> <p>b) All horizontal stay shall be of 25.4mm OD, 18SWG</p> <p>c) Supported with non-rusted 200mm x 50mm OD, noiseless smooth moving PU Wheels (04No) with double bearing &amp; double lock arrangement to each wheel.</p>
3	<b>Removable Stretcher Top :</b>	<p>a) Stretcher should be removable from trolley.</p> <p>b) Top - S.S. 18SWG Sheet, dished horizontally in middle.</p> <p>c) Stretcher dished sheet should be fitted on 25mm OD, 16SWG SS. Tube.</p> <p>d) Three Additional 31.7 x 6 mm S.S. stiffeners should be fully argon welded to main frame, to support S.S. dished top from underneath widthwise.</p> <p>e) Four legs - S.S. 25mm OD, 16SWG SS. tube having 190mm height fitted rubber bush.</p> <p>f) Push Handle at both ends 25mm OD, 16SWG SS. Tube &amp; covered with PVC Sleeves.</p>
4		<b>Govt. of Maharashtra Public Health Dept. &amp; Mfg date"</b> must be embossed at visible sight of frame & removable stretcher, must be easily readable
5	<b>Finish :</b>	<p>a) All S.S. should be deep fully argon seamless welded and polished finished.</p> <p>b) Tow section tops should be smooth edges and burr free and corners should be round off so that there should be no sharp corners.</p>
6	<b>General Requirements:</b>	<p>a) All stainless steel sheet &amp; stainless steel tubes/pipes used in manufacturing shall be of 304 S2 grade confirming to IS 6911 of 1992 or latest.</p> <p>b) All dimensions will be considered — Length, Width, Height in millimeter(mm), thickness in gauge (SWG — Standard Wide Gauge), Diameter should consider as Outer Diameter (OD).</p> <p>c) The stretcher trolley must be sturdy, vibration free and self balance.</p> <p>d) The stretcher trolley shall be properly constructed with all welded joints grounded, cleaned and well-formed. Unless otherwise specified, the vertical members shall be perpendiculars to the wheel base and parallel to each other and the horizontal members shall be at right angles to the vertical members.</p> <p>e) The stretcher trolley shall stand on all the legs at the same time on a level surface. All the surfaces shall be smooth and</p>

*Handwritten signature*  
10/6/19

*Handwritten signature*  
12/6/19  
Civil Dept

*Handwritten signature*  
Biomedical Engg.  
RRSH, Amravati

*Handwritten signature*  
RRSH, Amravati

		<p>free from pitting. Welding shall fully penetrate and shall be sound in every detail and it shall be finished flush. In the finished stage, there shall be no exposed sharp edges in the frame-work or other unsealed formations which may harbor dirt or foreign matter.</p> <p>f) The sketch shown in the specification is only indicative for the bidder.</p> <p>g) should attached inbuilt small cyliner trolley</p> <p>h) Tender committee has reserved rights to change dimensions &amp; sketch at any stage of tender.</p>
--	--	-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Wanted  
 Dr. Vinaya  
 Ambare  
 a.s.m.c, Mumbai

Dr. N. Rajeev  
 Thane Civil Hosp  
 13/6/19.

Amol  
 Amol Wadekar  
 Biomedical Engg.  
 RRSH, Amravati

Ramdas  
 13/6/19  
 K. M. Hospital  
 Mumbai



## Technical Specification of Wheel Chair

1	Overall Length :-	1050 mm Width : 680mm. Height : 910mm
2	Seat Height from floor at the front :	500mm.
3	Seat Height from floor at the back :	450mm
4	Arm Height from seat :	225mm.
5	Seat :	Length : 430mm Width between armrest pipes: 430mm
6	Back- Height :	380mm, Width at seat level : 430mm. Width at the Top: 430mm.
7	Clearance of footrest to floor :	90 to 200mm
8	Back Clearance of frame to floor:	100mm
9	Mean Rim Diameter :	500mm
10	Front Ringing :	Foldable cast aluminum foot res& 200mm OD Strong swiveling PU wheels, double bearing, provided in front
11	Rare Axel :	single position 12mm
12	Rare Wheel :	solid rubber tyre wheels-02 Nos, for self propulsion to hoops of 15.8mm OD, 18SWG tube, mounted on rims, with brake facility.
13	Material of frame :	25.4mm OD, 18SWG round tube, S.S.
14	Seat & Back :	18SWG, S.S.
15	Finish:	All section tops should be smooth edges and burr free and corners should be round off so that there should be no sharp corners
16	General Requirements:	<p>a) All stainless steel sheet &amp; stainless steel tubes/pipes used in manufacturing shall be of 304 S2 grade confirming to IS 6911 of 1992 or latest.</p> <p>b) All dimensions will be considered — Depth, Width, Height in millimeter(mm), thickness in gauge (SWG — Standard Wide Gauge), Diameter should consider as Outer Diameter (OD).</p> <p>c) The wheel chair must be sturdy, vibration free and self balance.</p> <p>d) The wheel chair shall be properly constructed with all welded joints grounded, cleaned and well-formed Unless otherwise specified, the vertical members shall be perpendiculars to the wheel base and parallel to each other and the horizontal members shall be at right angles to the vertical members.</p> <p>e) The wheel chair shall stand on all the wheels at the same time on a level surface. Welding shall fully penetrate and shall be sound in every detail and it shall be finished flush. In the finished stage, there shall be no exposed sharp edges in the frame-work or other unsealed formations which may harbor dirt or foreign</p>

Dr. Vinay  
Arbore  
C.A.M.C., Mumbai

Dr. N. R. R. R. R.  
Thane Civil Hosp  
Reg No 5313  
13/6/19.

Arul  
13/06/19  
Arul Wadkar  
Biomedical Engineer  
RRSH, A. Madhavli

Arul  
13/6/19  
RRSH, A. Madhavli

	<p>matter.</p> <p>f) The sketch shown in the specification is only indicative for the bidder.</p> <p>g) Tender committee has reserved rights to change dimensions &amp; sketch at any stage of tender.</p> <p>h) "Govt. of Maharashtra Public Health Dept. &amp; Mfg date" embossed plate must be riveted at visible sight, Embossed font can easily readable.</p>
--	--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

Dr. N. C. Rofade  
 Thane Civil Hosp  
~~13/6/19~~ 13/6/19.

Vinayak  
 Dr. Vinayak Ambekar  
 ACME, Mumbai.

Pranali  
 Dr. Pranali  
 13/6/19  
 KEM Hospital  
 Mumbai

Anil  
 Anil Wadhwa  
 Biomedical Engg  
 RRSH, Amravati

## Technical Specification of Examination Table with Foot Step

1	Clinical purpose	An examination table on which the patient lies during a examination. This table is usually found inside the examination room in hospital.
2	Used by clinical department/ward	Examination room
3	Technical characteristics specific to this type of device)	<ol style="list-style-type: none"> <li>1) Over all Size 1820 -1830mm Length x 600-610mm Width x 750-760mm Height</li> <li>2) All mild steel sheet used shall be CRCA quality.</li> <li>3) Two section table top CRCA 18SWG, all side double bent &amp; fixed on tubular frame.</li> <li>4) The table top have perennial recess made from 18SWG CRCA Sheet &amp; SS box to leg end with "C" channel sliding,</li> <li>5) Complete with the pair of SS lithotomy rods made from 12mm Dia SS 304 Grade, round bars with rexin ankle straps insert gear arrangement.</li> <li>6) The top should be support of 31 x 35 x 2mm made from CRCA sheet one side having. support of 31 x 3mm to receive the back section.</li> <li>7) The back section shall have 18 SWG CRCA Sheet in double bent at three sides &amp; one side closed beading having support must be provided with 25 x 5mm HR flat having welded to the support flat.</li> <li>8) A ratchet flat shall be provided to wit MS Support rods 3/8".</li> <li>9) The head flap adjustable on several indications both up &amp; down &amp; by easily accessible racj.</li> <li>10) Head &amp; Foot end welded tubular frame work made od 31.70D X 18SWG tube for vertical &amp; 25.5mmOD X 18 SWG horizontal.</li> <li>11) Gap between two legs must be 950-960mm lengthwise &amp; 520-530mm widthwise.</li> <li>12) Legs must be fitted with rubber shoes nylon inserts.</li> <li>13) One drawer 12 " x 15 " with reversible channel fitting, centrally locked with 3 keys.</li> <li>14) Aluminum top antiskid step stool having two steps.</li> <li>15) Suitable mattress 25 mm thick &amp; pillow should be tear proof covered with non pinching Rexine, seamless joint, washable and water-proof, having welcrow for fixing on table top --Qty 02 No.</li> <li>16) All components shall be thoroughly pre-treated chemically to remove rust &amp; foreign matters like grease, oil etc by deep tank seven process, including separate degreasing, derusting, phosphating each followed by water rinsing &amp; hot air drying to give phosphate coating confirming IS 3618-1966 class C. The treated metal surface should then be coated with epoxy polyester powder with paint film thickness of 60 microns &amp; oven baked at 180-210°C. This finish should exclude stainless steel parts, some hardware, ebonite rubber if any.</li> </ol>

*Pranav  
13/6/19  
Kamthambal  
Mumbai*

*Dr. N. K. Kulkarni  
Thane  
13/6/19*

*Amol Wadkekar  
Biomedical Engineer*

*Amol Wadkekar  
Biomedical Engineer  
R. R. S. H. Amravati*

*Dr. S. K. Kulkarni  
MORRI Amravati*

## Technical Specification of Attendant Stool

1	Overall Size :-	305mm (L) X 305mm(W) X 545mm(H) Height from Ground level to top.
2	Top & Frame :	<p>a) Top S.S. Sheet 18SWG, double bend at each side, mounted on frame structure</p> <p>b) Frame — S.S. tubular 25mm x 25mm, 18SWG</p> <p>c) All legs must provide neoprene rubber shoes.</p> <p>d) "Govt. of Maharashtra Public Health Dept &amp; Mfg date" must be embossed at visible sight, must easily readable.</p>
3	Finish :	<p>a) All S.S. should be deep fully argon seamless welded and polished finished.</p> <p>b) Tow section tops should be smooth edges and burr free and corners should be round off so that there should be no sharp corners</p>
4	General Requirements:	<p>a) All stainless steel sheet &amp; stainless steel tubes/pipes used in manufacturing shall be of 304 S2 grade confirming to IS 6911 of 1992 or latest.</p> <p>b) All dimensions will be considered — Length, Width, Height in millimeter(mm), thickness in gauge (SWG — Standard Wide Gauge), Diameter should consider as Outer Diameter (OD).</p> <p>c) The stretcher trolley must be sturdy, vibration free and self balance. <b>ATTENDANT STOOL</b></p> <p>d) <del>The stretcher trolley</del> shall be properly constructed with all welded joints grounded, cleaned and well-formed. Unless otherwise specified, the vertical members shall be perpendiculars to the wheel base and parallel to each other and the horizontal members shall be at right angles to the vertical members. <b>ATTENDANT STOOL</b></p> <p>e) <del>The stretcher trolley</del> shall stand on all the legs at the same time on a level surface. All the surfaces shall be smooth and free from pitting. Welding shall fully penetrate and shall be sound in every detail and it shall be finished flush. In the finished stage, there shall be no exposed sharp edges in the frame-work or other unsealed formations which may harbor dirt or foreign matter.</p> <p>f) The sketch shown in the specification is only indicative for the bidder.</p> <p>g) Tender committee has reserved rights to change dimensions &amp; sketch at any stage of tender.</p>

*Dr. N. W. Wadekar*  
 13/6/19

*Dr. N. W. Wadekar*  
 Thane Civil Hosp  
 13/6/19.

*Amol Wadekar*  
 Biomedical Engineer  
 R.R.H. Amravati

*Dr. R. R. Amavadi*  
 (Dr. R. S. Khobragade)

*Dr. V. V. Amavadi*  
 G. A. M. Amavadi